

TEST REPORT

Searchable via: <https://brown-biology.com/>



Contact at: Admin@brown-biology.com

Task Number > #6409262 Received Date > May 08,2026

COA Key > 6409262 Reported Date > May 12,2026



Authentic Results
results shall be open and transparent.



Accurate Reports
Accurate data.verified multiple times



Quality You Can Trust
Rigorous testing. Reliable results.

Sample Semax 30mg Batch 40926


Sample description > Tests requested >

See picture or pictures attached.



Assessment of a peptide vial or vials.

Specification	Result	Method	Status
Identity: Semax	Semax	MALDI-MS	✓ Conforms
Content	30.13 mg	HPLC Quantitation	✓ Conforms
Overall Purity	99.64%	RP-HPLC (214 nm)	✓ Conforms

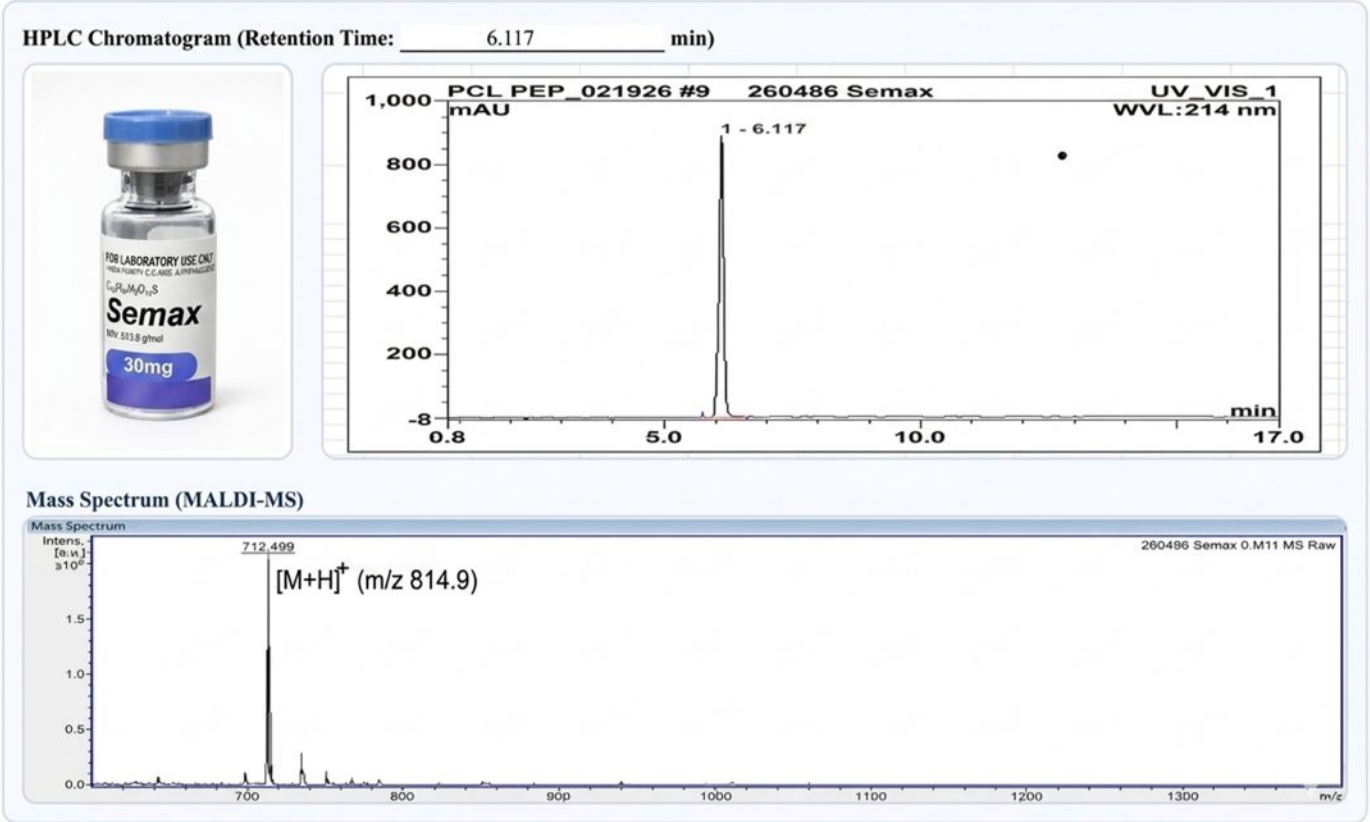

Research and Formulation Chemist

Bisbanz

This purity analysis was conducted using UPLC/MS under standard laboratory conditions, following validated analytical protocols to ensure accurate and reliable results. This analysis is intended for informational and research applications.